

File D:\DATA\BACKUP\RAWDATA\

Injection Date : 23-May-14, 17:02:13

Sample Name : 248

Acq. Operator : Monitor

Spec. Reported : MS Integration

Acq. Method : D:\METHODS\HPLC.M

Analysis Method : D:\METHODS\1-POS-3MIN.M

Sample Info : Easy-Access Method: 'HPLC'

Method Info : Mobile Phase : A: Water (10mM NH₄HCO₃) B: Acetonitrile

Gradient : 5%B increase to 95%B within 1.3min,

95%B for 1.5min, back to 5%B within 0.01min.

Flow Rate : 1.8mL/min

Column : XBridgeC18, 4.6*50mm, 3.5um

Column Temperature : 50 C

Tgt Mass (EZX) :


Location : P1-E-01

Inj : 0


Inj Volume : 1.2 ul

Detection: UV (214, 4nm) and MS (ESI, Pos mode, 110 to 1000amu)


ADC1 A, ELSD

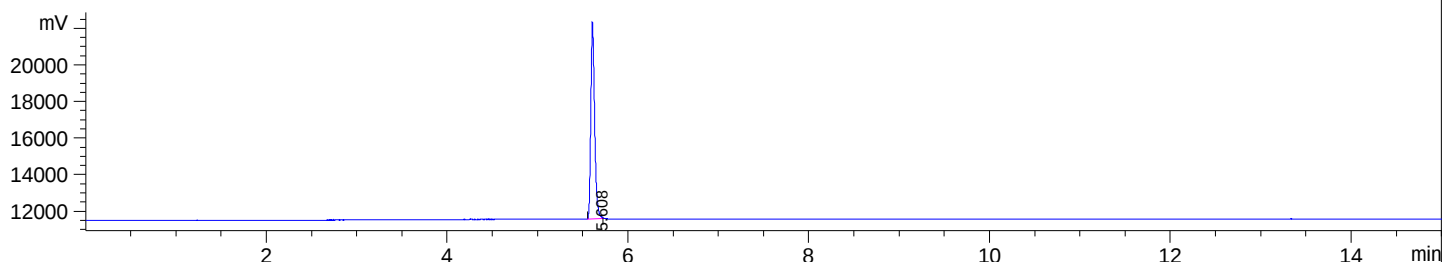

DAD1 A, Sig=214,4 Ref=off

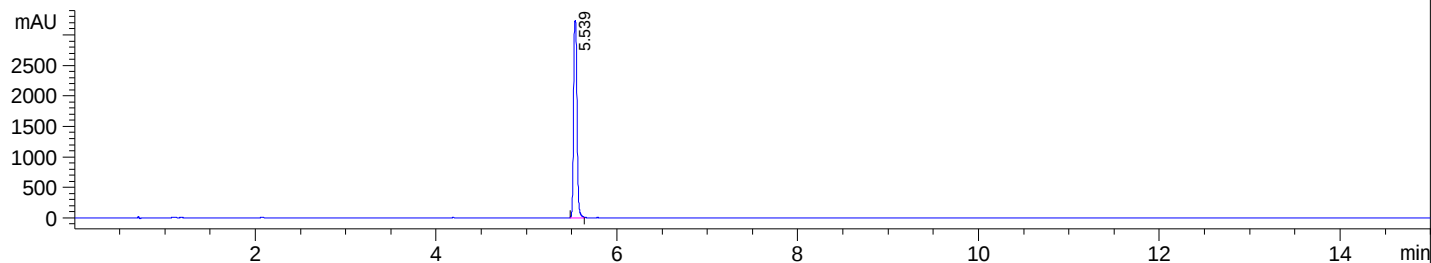

DAD1 B, Sig=254,4 Ref=off

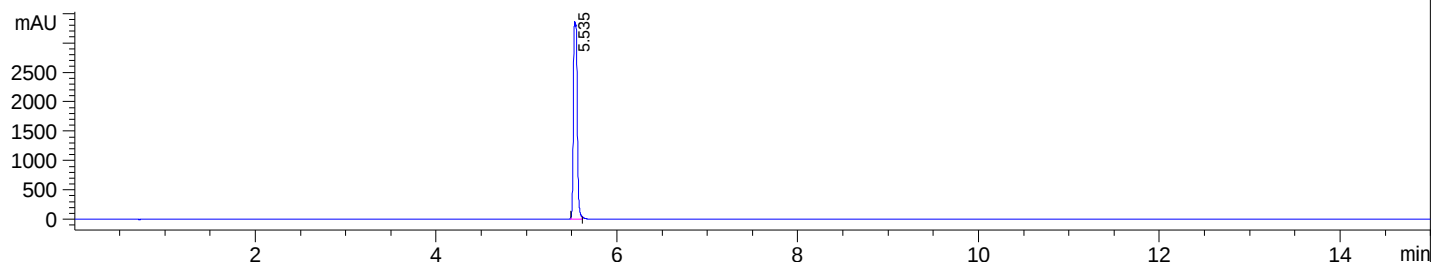

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
5.61	0.04	31403.93	10767.32	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
5.54	0.04	8571.35	3236.01	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
5.54	0.04	9846.39	3359.45	100.00